

mRNA Detection with Fluorescence-base Imaging Techniques for Arthritis Diagnosis

Anne Yau^{1,2}, Hongchuan Yu³ and Yupeng Chen^{1,2*}

¹Department of Biomedical Engineering, University of Connecticut, Storrs, CT 06269, USA

²Department of Orthopedics and Department of Molecular Pharmacology, Physiology and Biotechnology, Brown University, Providence, RI 02903, USA

³Dicerna Pharmaceuticals, Cambridge, MA 02140, USA.

Received February 26, 2018; Accepted February 28, 2019; Published July 16, 2019

Keywords: mRNA detection, Fluorescence, Diagnosis, Arthritis

INTRODUCTION

Arthritis is a term used to indicate joint pain that are caused by inflammation of joints or joint disease that occur commonly among older people. People of all ages, sexes and race can and do have arthritis as well. There are different types of arthritis with different causes and treatment methods but the most commonly known are the Rheumatoid Arthritis (RA) and the Osteoarthritis (OA). The symptoms of arthritis are joint pain, swelling, stiffness and decreased range of motion which could develop over time or appear suddenly. These symptoms may or may not exacerbate over time. As the disease get more severe, it could prevent patients from doing daily activities such as walking up the stairs and experience chronic pain [1].

There are multiple approaches for diagnosing arthritis other than performing physical examinations by the doctor or rheumatologists. Conventional radiography (CR) is one of the many imaging methods for diagnosis. CR is cheap compared to the alternative, magnetic resonance imaging (MRI) and faster than ultrasound. However, CR can only be used towards the end of the disease process, where the bones have eroded and joint spaces narrowing [1] and it does not show soft tissue sufficiently [2]. Both ultrasound and MRI are not favorable due to the time it takes for diagnosis with ultrasound and the high cost in exchange for high sensitivity of MRI. Positron emission tomography (PET) has made its way into diagnosing the disease for its high sensitivity detection and potential for whole-body evaluation [3]. However, due to the short half-life of some isotopes used for this technique, patients will mostly be subjected to radiation exposure which may cause more health problems in the future. Optical imaging (OI) have been around in the microscopic world is now making its way to the macroscopic setting where this technique offers high sensitivity for detection of inflammation [4,5], fast and inexpensive and most importantly do not expose patients to

ionizing radiation [3]. OI is perfect for detecting and diagnosing rheumatoid arthritis that mainly affects small joints of hands and feet. Many medical equipment, such as the X-ray radiography, computed tomography (X-RAY CT), radionuclide imaging using single photons (Single Photon Emission Computer Tomography SPECT) and positrons (Positron Emission Tomography PET), magnetic resonance imaging (MRI), ultrasonography (US) and optical imaging require 'contrast agents' for the extraction of information of the human bodies [6,7]. Real-time PCR, fluorescence *in situ* hybridization (FISH) analysis have been widely used at the cellular level to detect expression levels and cell distribution of mRNA [8].

Examples of contrast agents are the super paramagnetic or paramagnetic metals, such as Gadolinium Contrast Medium, used in MRI that mainly observed the whole-body scan. To get a more target specific imaging, molecular imaging such as PET and optical imaging like fluorescence microscopy are used for their sensitivity and specificity for target detection. However, the disadvantages uses of PET are that they have poor spatial and temporal resolution. They also require radioactive compounds that have intrinsically limited half-life which limit their repeated use due to safety regulation [9,10]. In this review, we will focus on detecting mRNA at real-time with fluorescence microscopy and the diagnosis of arthritis with fluorescence-based imaging

Corresponding author Yupeng Chen, PhD, Associate Professor, Department of Biomedical Engineering, University of Connecticut, 260 Glenbrook Road, Unit 3247, Storrs, CT 06269-3247, USA, Tel: 860-486-7911; Fax: 860-486-2500; E-mail: yupeng.chen@uconn.edu

Citation: Yau A, Yu H & Chen Y. (2019) mRNA Detection with Fluorescence-base Imaging Techniques for Arthritis Diagnosis. *J Rheumatol Res*, 1(2): 39-46.

Copyright: ©2019 Yau A, Yu H & Chen Y. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

techniques.

FLUORESCENCE-BASED IMAGING TECHNIQUES

In the past few centuries, there was a surge in the use of fluorescent dye in various areas. Special dyes are used for printing valuable documents such as money, and certificates. Some dyes are used to aid in leak detections of oils and fluids in vehicles. Because of its distinct ability, the dyes are also used to assist in exploration of water underground. Using similar concept in large scale, researchers started to apply this approach in *in vivo* medical imaging. Despite countless of organic dyes in the market for research, there are only two fluorophores that's approved by the US Food and Drug Administration (FDA) for medical use, which are the fluorophores are indocyanine green (ICG) and fluorescein [11-13]. ICG is used as an ophthalmologic agent and as a hepatic functional agent while fluorescein is used primarily in ophthalmology. These two agents, with no toxicity reported, are primarily used to obtained retinal angiograms that require high dosage of the agents. Even though fluorophores dyes in optical imaging have made great strides in the imaging field, an ideal labeling reagent would be the ones that remain non-fluorescent until bound to its target.

Fluorescence microscopy, providing real-time visualization in the surgical field, has similar sensitivity to radionuclide imaging, providing high resolution, high contrast, high specificity and quantitative of the sample. The downside of optical imaging is that uncertainty emerges as the scans get into deep tissue due to unpredictable light scattering and absorption [14,15]. Hence, the best place to use optical imaging is on the superficial tissue surfaces such as the breasts or the lymph nodes [16-20]. However, with the continued growth in the medical imaging techniques, dyes used for contrast images have improved significantly.

To obtain a successful optical molecular probe for medical imaging, the right wavelength must be employed to excite the dye to obtain a unique emission wavelength. However, if the excitation wavelength is near the ultraviolet region, the tissue will be damaged, while excitation on at the infrared region will cause tissue heating. Absorbance and auto fluorescence could be observed in any case when there is asymmetrical stokes shift [12]. To prevent the auto fluorescence by the tissue under low interference, many researchers and scientists have started applying light in the near-infra red (NIR) wavelength (650-900 nm) as the excitation energy. These NIR wavelengths are invisible to

human eyes [21]. The incorporation of NIR fluorophores with current optical imaging techniques provides an intraoperative image-guided surgery that allows for target-specific imaging due to ultralow background auto fluorescence [15].

Previous study of OI have shown promising results after injection of fluorescent dyes for detection of arthritis [4,5,22,23]. Another study has successfully shown that *in vivo* leukocyte cell can be tracked by using optical imaging techniques. These *in vivo* leukocyte cells are labeled with fluorescent dyes, which are suitable for the detection of synovial inflammation in an antigen-induced arthritis model [3].

There are few available fluorescence-based imaging techniques: fluorescence microscopy, flow cytometry, cell sorting fluorescence correlation spectroscopy as well as particle tracking velocimetry [7].

Visualization mRNA with different hybridization methods

FISH: The localization of mRNA in cell has been around since 1980s, but then, mRNA translation could only be visualized via *in situ* hybridization (ISH) using probes with multiple fluorophores or multiple probes with one fluorophore [24]. The groups have succeeded in transcript detection *in situ*, enabling genotyping of individual transcript molecule. The earliest single molecular RNA imaging studies was transcribed and fluorescently labeled *in vitro* [25]. As seen in **Figure 1A**, hybridization-based methods for RNA imaging are as shown. Fluorescence *in situ* Hybridization (FISH) can differentiate RNA molecules with just a single base because it only binds to specific parts of the nucleic acid. FISH are convenient procedures due to its highly sequence-specific when combined with amplifications during procedures in fixed cells [26,27]. Not only FISH can detect and localized RNA targets in cells, cancer cells and tissues, it also assists in defining dimensions of gene expression in cells and tissues in addition to exploring cell reproduction cycle. The fluorophores are usually attached to a strand analogous to its target and in FISH, the progress of the probes can be observed from the very beginning to the end, when it reaches its target, because of its fluorescence nature. It is also important to note that the probe size must be small enough to complement the target, and that multiple colored probes (with different wavelengths) can be used together.

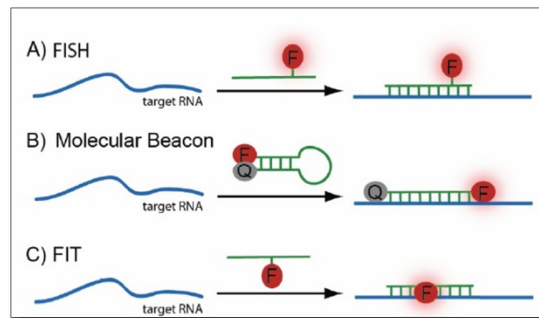


Figure 1. Three different hybridization techniques. (A) Fluorescence *in situ* hybridization (FISH) consists of a DNA strand analogous to its target together with a fluorescence dye. (B) Molecular beacon (MB) is a hairpin like structure that has a quencher on the 3' end and reporter dye on the 5'. When it reaches the target, the hairpin opened, separating the fluorophore and dye enabling fluorescence. (C) Forced intercalation (FIT). The fluorophores with DNA strand similar to its target is only enabled when it binds with the target.

Molecular beacons: Molecular beacons (MB) have been used in variety of applications involving real-time mRNA detection in living cells [28], DNA-RNA hybridization studies and protein/DNA interactions [29]. MB, as seen in **Figure 2**, is a hairpin-like oligonucleotides probe consisted of single-stranded DNA molecule in a stem-loop conformation with a fluorophore linked to 5' end and a

quencher at the 3' end with a minimal distance from each other. When the molecular beacon reaches its target, the hairpin-like structure then stretches out, separating the fluorophore and quencher, enabling fluorescence, with about 100 times more intensely than background levels of unbound probes.

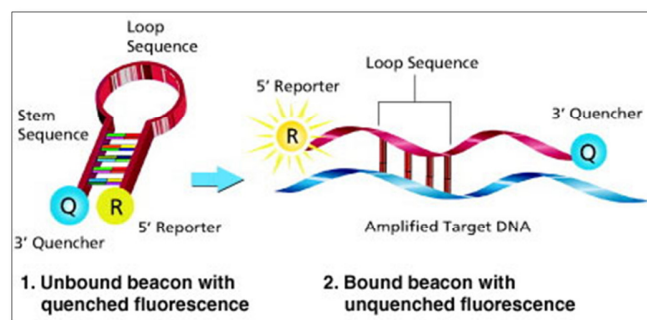


Figure 2. Molecular beacons used in applications involving real-time mRNA detection in living cells. The hair-pin like structure is equipped with 3'quencher and 5'reporter which is an organic dye. Once the beacon reaches target, it will open up, enabling fluorescence.

An example for the success of molecular beacon is explained in a paper published in 2011 by Bratu et al. [29]. Molecular beacons in the paper are synthesized from modified nucleic acids (2'-O-methyl RNA and DNA) to increase target specificity and sensitivity and labeled with various fluorophores and specific quenchers respectively as seen in **Tables 1 and 2**. They concluded that they were able to

synthesize small MB from 2'-O-methyl RNA/LNA chimeric nucleic acids and these hairpins are observed to be stable in cellular environment and high affinity for binding to target RNAs. They also demonstrated that different fluorophores can be used to make the tiny MB which aided in detecting highly structured RNAs, small RNAs and microRNAs which can be seen in **Tables 1 and 2**.

Table 1. Fluorophore labels for molecular beacon probes.

Fluorophore	Alternative Fluorophore	Excitation (nm)	Emission (nm)
TMR	Alexa 546*, Cy3**	555	575
Texas Red	Alexa 594*	585	605
Cy5b	Alexa 647*	650	670

* Alexa fluorophores are available from Invitrogen

**Cyanine dyes are available from Amersham Biosciences

fluorescent dyes [7]. Other than *in vivo* targeting and imaging, QDs are also used in cellular targeting and imaging, as well as fixed tissue analysis, optical encoding and quantitative determination [33].

Size of the quantum dot nanoparticles in bioimaging field generally falls within 2-10 nm in diameter. QDs have unique optical and electronic properties, with molar extinction coefficients that are 10-50 times larger, making it much brighter than conventional dyes. The emission wavelengths are size tunable depending on the radius of the QD. Larger QDs were also synthesized to be used in other applications other than *in vivo* imaging. However, parameters such as the distance between gold nanoparticle to optical absorbance and scattering intensity of the inter-particle distance can be controlled, resulting in a research group utilizing 20 nm Au nanoparticles QD to predict the localized surface plasmon resonance (LSPR) of gold nanoparticles. They were able to synthesize 20 nm AuNP monomers with zero LSPR background as probes with only a single target molecule required to form a dimer with significant plasmon resonance coupling effect, increasing the sensitivity of the LSPR sensor to single cell level. In their study, they were able to present a smart single mRNA imaging approach in living cells based on target-induced formation of nanoparticle dimers. They concluded that with proper linker, these nanoparticles could

serve as a basis to many imaging techniques for biomolecules and mRNA in living cells [34].

The optical properties of quantum dots originated from their elemental composition, with a semiconductor core such as cadmium selenide (CdSe) or lead selenide (PbSe), coated with a semiconductor shell, as seen in **Figure 4**. Properties of QDs have made an impression in the optical imaging field, prompted a topic of intensive interest in cancer biology, molecular imaging and molecular profiling [32,35-42]. Although QDs presented the researchers numerous advantages over traditional organic dyes, these inorganic semiconductor materials are toxic to living systems, limiting their use in biological systems, triggering a hot topic for research in the field on synthesizing a more biocompatible QD for the biological systems. Multiples experiments have been conducted on modified QDs, such as extra surface coating to minimize the cytotoxicity [32]. For example, cadmium ions present in the many QDs are shown to bind to thiol groups on important molecules in the mitochondria causing cell death [32]. The cadmium ions present in the cells are most likely caused by QD exposure to air and UV light, causing the surface to oxidize in oxidative solution. The levels of cytotoxicity could be reduced or eliminated by addition surface coatings [32].

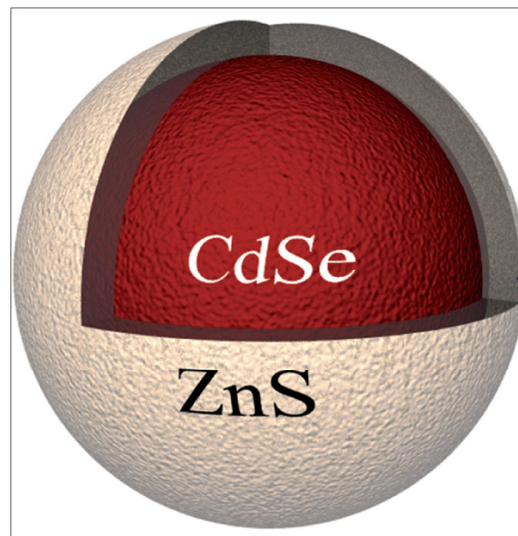


Figure 4. Quantum Dots of CdSe core with ZnS shell.

QUANTUM DOTS and MOLECULAR BEACONS: Since quantum dots have become interesting fluorophores for biological imaging fields, researchers have developed a new method for the fluorescence imaging of endogenous mRNA using signal-tunable molecular beacon technique based on QDs in living cells. As seen in **Figure 5**, the group targeted mRNA124a which was observed to have high expression during neuronal development [43]. The beacons, each composed of a quencher on the mRNA124a binding sequence and the R9 peptide, are incorporated with a

quantum dots to form R9-QD-mRNA124a beacon. In the absence of mRNA124a, R9-QD-mRNA124a formed a partial duplex beacon that quenches the system, giving no fluorescence signal. With mRNA124a, the mRNA124a binding sequences leave together with the quenchers, leaving a signal of red fluorescence. They concluded that the method could provide critical information on expression during neurogenesis and could be applied to various systems to track cellular developments with different sized QD-based molecular system.

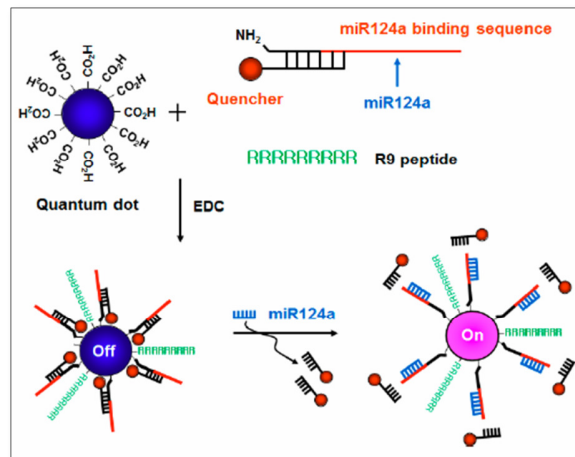


Figure 5. Schematic of R9-QD-miR124a beacons to image miR124a. The oligonucleotide consists of an amine end and a quencher with miR124a recognition sequence. The carboxylated QD was combined with the oligomer and R9 peptide to create R9-QD-miR124a.

CONCLUSION

There are many restrictions obtaining multicolor *in vivo* imaging mainly due to overlapping fluorescence emissions. Different approaches have been executed, including the recently developed 3'untranslated region (UTR)-based reported gene imaging system to monitor the expression of patterns of mRNA. However, with this approach, it is difficult to differentiate if the data obtained are from the mRNA expression or from cell death *in vivo* [44-47].

On the other hand, different fluorophores with discernable emissions wavelength must be chosen for multicolor imaging. The complications for the traditional dyes such as organic dyes and QDs are the requirement to use UV or short-wavelength radiation for excitation of the materials and their cytotoxicity in biological environment. Low light penetration depth is observed due to the short wavelength excitation light or low signal-to-noise ratio due to auto-fluorescence. Although fluorescence-based imaging techniques have improved tremendously, there are still rooms to improve the techniques or the probes. It is important to develop more efficient bio-labels to overcome these limitations. NIR probes have gained its momentum the past decades to overcome the shortcomings of the traditional probes when it comes to monitoring the sample with higher depth. Few companies have developed some NIR fluorophores with emission >800 nm, permitting NIR probes to be used together with the original fluorescent organic dye [48]. With the developments of new types of contrast agents together with improvement in electronics and software in equipment, fluorescence-based imaging technique can expand even more. In conjunction of NIR probes, quantum dots have also been an interesting tool not only for imaging field, but for the computing as well as the quantum dot displays for lightning up LCD displays in televisions. Many researches could be done in terms of quantum dots in the

field of nanotechnology. Future work such as incorporating the reporter tag into endogenous gene loci using CRISPR-Cas0 genome editing tools would proof to be quite interesting [49].

The NIR dye, ICG, is already being used to test for liver cancer during surgery, to identify small and unidentifiable liver cancers in real time. ICG has also been used to identify lymph nodes in real time in a small number of breast cancer patients [50]. Even though optical imaging has yet to replace conventional imaging as a form of arthritis tool, OI is a promising diagnostic tool for detecting early onset arthritis.

In summary, this review analysis on the visualization of mRNA with different hybridization techniques. There were many shortcomings since the development of fluorescence-based imaging techniques, but scientists and researchers have all overcome the obstacles and improved both the probes and instruments for a better future. The capability of fluorescence-based imaging techniques is open to new possibilities for better and faster diagnostic of joint diseases in the future.

CONFLICT OF INTEREST

Dr. Yupeng Chen is a co-founder of NanoDe Therapeutics, Inc.

ACKNOWLEDGEMENT/FUNDING

We would like to thank our funding supports: R03AR069383-01 (NIH), 1R01AR072027-01 (NIH), and Faculty Early Career Development (CAREER) award (1653702) from NSF.

RÉFERENCES

1. Golovko D, Meier R, Rummenny E, Daldrup-Link H (2011) Optical imaging of rheumatoid arthritis. *Int J Clin Rheumtol* 6: 67-75.

2. Roemer FW, Crema MD, Trattnig S, Guermazi A (2011) Advances in imaging of osteoarthritis and cartilage. *Radiology* 260: 332-354.
3. Simon GH, Daldrup-Link HE, Kau J, Metz S, Schlegel J, et al. (2006) Optical imaging of experimental arthritis using allogeneic leukocytes labeled with a near-infrared fluorescent probe. *Eur J Nucl Med Mol Imaging* 33: 998-1006.
4. Chen WT, Mahmood U, Weissleder R, Tung CH (2005) Arthritis imaging using a near-infrared fluorescence folate-targeted probe. *Arthritis Res Ther* 7: R310-R317.
5. Wunder A, Tung CH, Muller-Ladner U, Weissleder R, Mahmood U, et al. (2004) *In vivo* imaging of protease activity in arthritis: A novel approach for monitoring treatment response. *Arthritis Rheum* 50: 2459-2465.
6. Kobayashi H, Ogawa M, Alford R, Choyke PL, Urano Y, et al. (2010) New strategies for fluorescent probe design in medical diagnostic imaging. *Chem Rev* 110: 2620-2640.
7. Kizek R, Ryvolova M, Chomoucka J, Drbohlavova J, Kopel P, et al. (2012) Modern micro and nanoparticle-based imaging techniques. *Sensors* 12: 14792-14820.
8. Soonhag K, Lee J, Moon SU, Lee YS, Ali BA, et al. (2015) Quantum dot-based molecular beacon to monitor intracellular microRNAs. *Sensors* 15: 12872-12883.
9. Schaeffter T (2005) Imaging modalities: Principles and information content. *Prog Drug Res* 62: 15-81.
10. Boswell CA, Brechbiel MW (2007) Development of radioimmunotherapeutic and diagnostic antibodies: An inside-out view. *Nucl Med Biol* 34: 757-778.
11. Jo D, Hyun H (2017) Structure-inherent targeting of near-infrared fluorophores for image-guided surgery. *Chonnam Med J* 53: 95-102.
12. Mondal SB, Gao S, Zhu N, Liang R, Gruev V (2014) Real-time fluorescence image-guided oncologic surgery. *Adv Cancer Res* 124: 171-211.
13. Merian J, Gravier J, Navarro F, Texier I (2012) Fluorescent nanoprobe dedicated to *in vivo* imaging: From preclinical validations to clinical translation. *Molecules* 17: 5564-5591.
14. Ntziachristos V, Funovics M, Weissleder R, Tung CH (2003) Protease sensors for bioimaging. *Anal Bioanal Chem* 377: 956.
15. Weissleder R, Tung CH, Mahmood U, Bogdanov A Jr. (1999) *In vivo* imaging of tumors with protease-activated near-infrared fluorescent probes. *Nat Biotechnol* 17: 375-378.
16. Ntziachristos V, Yodh AG, Schnall M, Chance B (2000) Concurrent MRI and diffuse optical tomography of breast after indocyanine green enhancement. *Proc Natl Acad Sci U S A* 97: 2767-2772.
17. Corlu A, Choe R, Durduran T, Rosen MA, Schweiger M, et al. (2007). Three-dimensional *in vivo* fluorescence diffuses optical tomography of breast cancer in humans. *Opt Express*. 15: 6696-6716.
18. Hawrysz DJ, Sevick-Muraca EM (2000) Developments toward diagnostic breast cancer imaging using near-infrared optical measurements and fluorescent contrast agents. *Neoplasia* 2: 388-417.
19. Kobayashi H, Hama Y, Koyama Y, Barrett T, Regino CA, et al. (2007) Simultaneous multicolor imaging of five different lymphatic basins using quantum dots. *Nano Lett* 7: 1711-1716.
20. Hama Y, Koyama Y, Urano Y, Choyke PL, Kobayashi H, et al. (2007) Two-color lymphatic mapping using Ig-conjugated near infrared optical probes. *J Invest Dermatol* 127: 2351.
21. Weil TT, Parton RM, Davis I (2010) Making the message clear: Visualizing mRNA localization. *Trends Cell Biol* 20: 380-390.
22. Hansch A, Frey O, Hilger I, Sauner D, Haas M, et al. (2004) Diagnosis of arthritis using near-infrared fluorochrome Cy5.5. *Invest Radiol* 39: 626-632.
23. Hansch A, Frey O, Sauner D, Hilger I, Haas M, et al. (2004) *In vivo* imaging of experimental arthritis with near-infrared fluorescence. *Arthritis Rheum* 50: 961-967.
24. Ainger K, Avossa D, Morgan F, Hill SJ, Barry C, et al. (1993) Transport and localization of exogenous myelin basic protein mRNA microinjected into oligodendrocytes. *J Cell Biol* 123: 431-441.
25. Larsson C, Grundberg I, Söderberg O, Nilsson M (2010) *In situ* detection and genotyping of individual mRNA molecules. *Nat Methods* 7: 395-397.
26. Paré A, Lemons D, Kosman D, et al. (2009) Visualization of individual Scr mRNAs during *Drosophila* embryogenesis yields evidence for transcriptional bursting. *Curr Biol* 19: 2037-2042.
27. Bratu DP, Cha BJ, Mhlanga MM, Kramer FR, Tyagi S, et al. (2003) Visualizing the distribution and transport of mRNAs in living cells. *Proc Natl Acad Sci U S A* 100: 13308-13313.
28. Perlette J, Weihong T (2001) Real-time monitoring of intracellular mRNA hybridization inside single living cells. *Anal Chem* 73: 5544-5550.
29. Bratu Diana P, Catrina Irina E, Marras Salvatore AE, Gerst JE (2011) RNA detection and visualization: Methods and protocols. *Methods Mol Biol* 714.

30. Singhal M, Sharma JK, Kumar S (2012) Effect of biocompatible glutathione capping on core-shell ZnS quantum dots. *J Mater Sci Mater Electron* 23: 1387-1392.
31. Köhler O, Jarikote DV, Seitz O (2005) Forced intercalation probes (FIT Probes): Thiazole orange as a fluorescent base in peptide nucleic acids for homogeneous single-nucleotide-polymorphism detection. *Chembiochem* 6: 69-77.
32. Walling MA, Novak JA, Shepard JRE (2009) Quantum dots for live cell and *in vivo* imaging. *Int J Mol Sci* 10: 441-491.
33. Li XL, Zhang ZL, Zhao W, Xia XH, Xu JJ (2016) Oriented assembly of invisible probes: Towards single mRNA imaging in living cells. *Chem Sci* 7: 3256-3263.
34. Baruah S, Ortinero C, Shipin OV, Dutta J (2012) Manganese doped zinc sulfide quantum dots for detection of *Escherichia coli*. *J Fluoresc* 22: 403-408.
35. Drummen G (2010) Quantum dots-from synthesis to applications in biomedicine and life sciences. *Int J Mol Sci* 11: 154-163.
36. Jin ZW, Hildebrandt N (2012) Semiconductor quantum dots for *in vitro* diagnostics and cellular imaging. *Trends Biotechnol* 30: 394-403.
37. Liu QH, Deng RP, Ji XL, Pan DC (2012) Alloyed Mn-Cu-In-S nanocrystals: A new type of diluted magnetic semiconductor quantum dots. *Nanotechnology* 23: 2-6.
38. Mattoussi H, Palui G, Na HB (2012) Luminescent quantum dots as platforms for probing *in vitro* and *in vivo* biological processes. *Adv Drug Deliv Rev* 64: 138-166.
39. Mukerjee A, Ranjan AP, Vishwanatha JK (2012) Combinatorial nanoparticles for cancer diagnosis and therapy. *Curr Med Chem* 19: 3714-3721.
40. Nie SM, Xing Y, Kim GJ, Simons JW (2007) Nanotechnology applications in cancer. In: *Annual Review of Biomedical Engineering*. *Annu Rev* 9: 257-288.
41. Pericleous P, Gazouli M, Lyberopoulou A, Rizos S, Nikiteas N, et al. (2012) Quantum dots hold promise for early cancer imaging and detection. *Int J Cancer* 131: 519-528.
42. Singhal M, Sharma JK, Kumar S (2012) Effect of biocompatible glutathione capping on core-shell ZnS quantum dots. *J Mater Sci Mater Electron* 23: 1387-1392.
43. Wu SM, Tian ZQ, Zhang ZL, Huang BH, Jiang P, et al. (2010) Direct fluorescence *in situ* hybridization (FISH) in *Escherichia coli* with a target-specific quantum dot-based molecular beacon. *Biosensors and Bioelectronics* 26: 491-496.
44. Ko MH, Kim S, Hwang DW, Ko HY, Kim YH, et al. (2008) Bioimaging of the unbalanced expression of microRNA9 and microRNA9* during the neuronal differentiation of P19 cells. *FEBS J* 275: 2605-2616.
45. Kim HJ, Kim YH, Lee DS, Chung JK, Kim S, et al. (2008) *In vivo* imaging of functional targeting of miR-221 in papillary thyroid carcinoma. *J Nucl Med* 49: 1686-1693.
46. Ko HY, Hwang DW, Lee DS, Kim S (2009) A reporter gene imaging system for monitoring microRNA biogenesis. *Nat Protoc* 4: 1163-1169.
47. Hsu PD, Lander ES, Zhang F (2014) Development and applications of CRISPR-Cas9 for genome engineering. *Cell* 157: 1262-1278.
48. Lee JY, Kim S, Hwang DW, Jeong JM, Chung JK, et al. (2008) Development of a dual-luciferase reporter system for *in vivo* visualization of MicroRNA biogenesis and posttranscriptional regulation. *J Nucl Med* 49: 285-294.
49. Wright AV, Nunez JK, Doudna JA (2016) Biology and applications of CRISPR systems: Harnessing nature's toolbox for genome engineering. *Cell* 164: 29-44.
50. Gompels LL, Lim NH, Vincent T, Paleolog EM (2010) *In vivo* optical imaging in arthritis - An enlightening future? *Rheumatology* 49: 1436-1446.